## This Page Is Inserted by IFW Operations and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**


Defective images within this document are accurate representations of the original documents submitted by the applicant.


Defects in the images may include (but are not limited to):


- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


## IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.

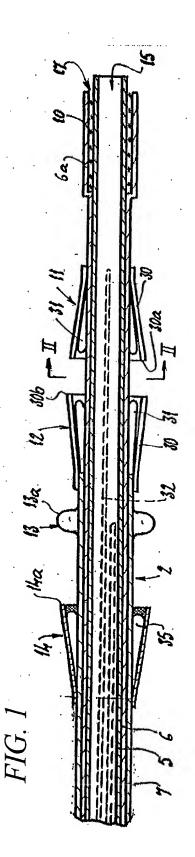


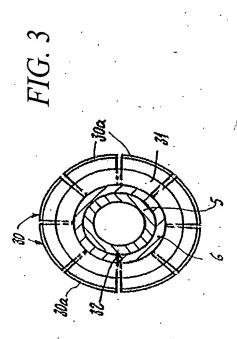



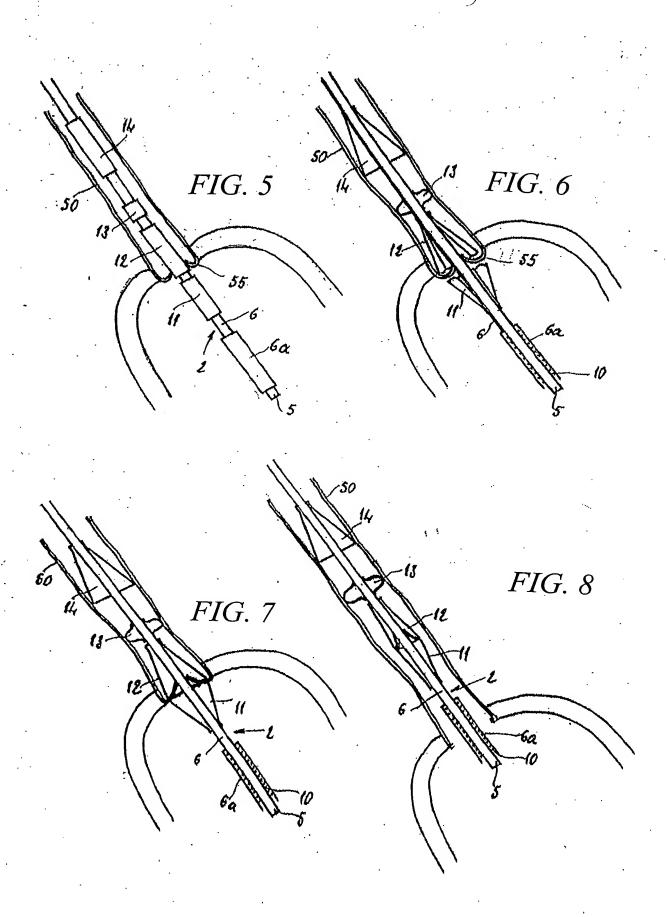

Appl. No.: Unknown

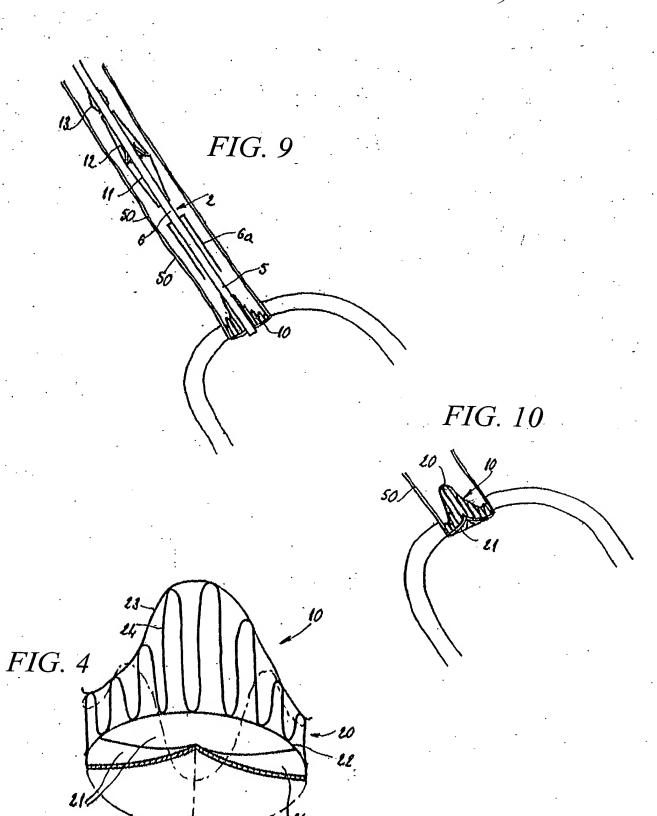

Appl. No.: Unknown



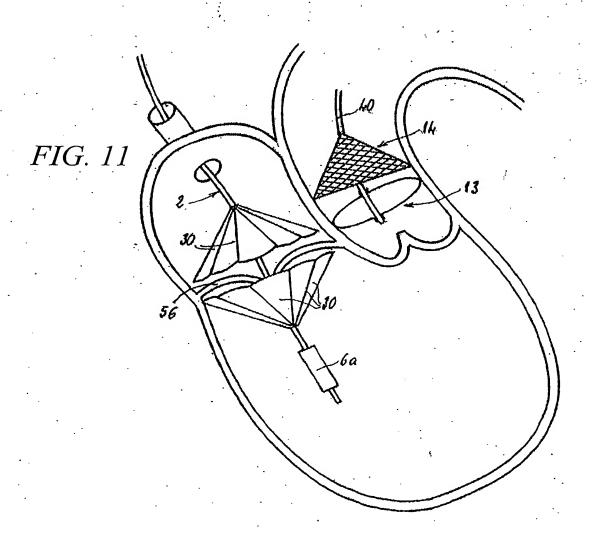



FIG. 12


Seguin, et al.
Appl. No.: Unknown Atty Docket: CVALVE.006CP1

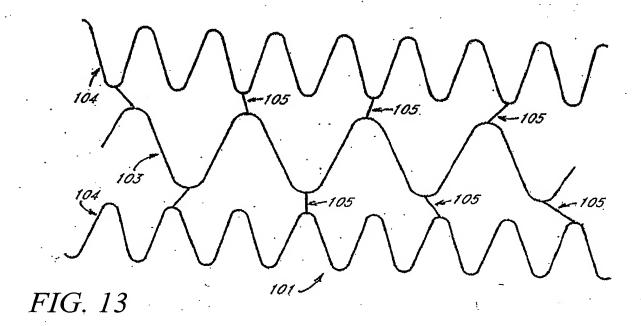

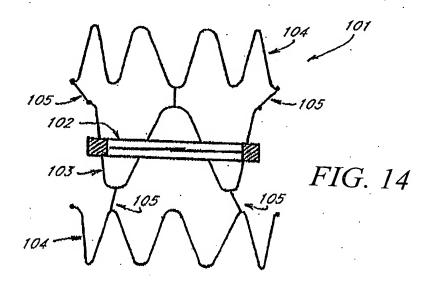


Appl. No.: Unknown

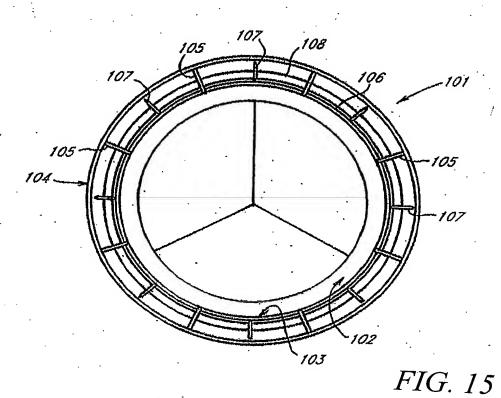

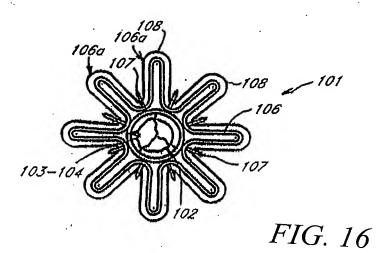

Appl. No.: Unknown

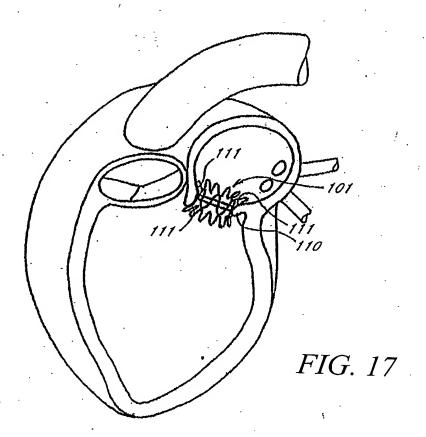

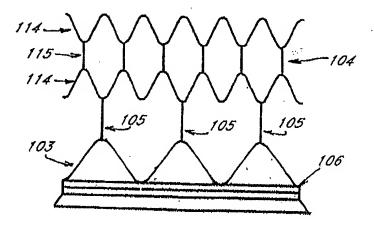


FIG. 18

Appl. No.: Unknown

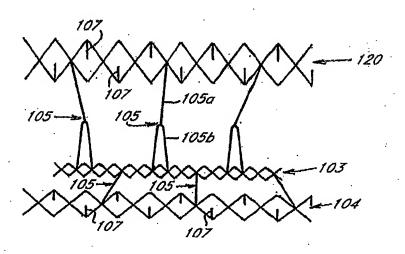


FIG. 19



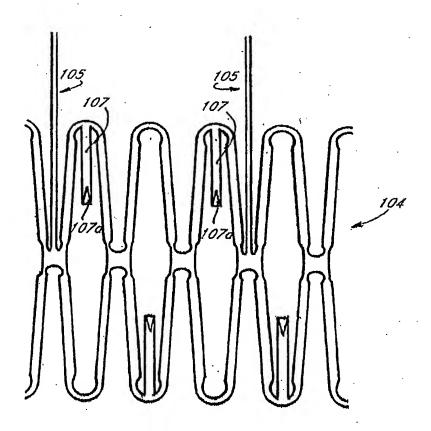


FIG. 20

Appl. No.: Unknown

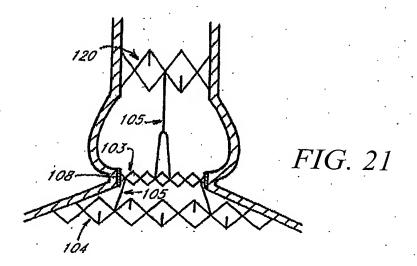


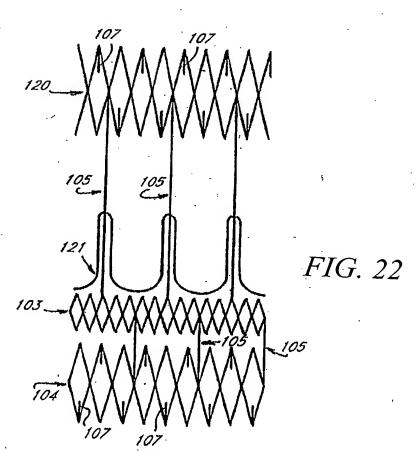


PROSTHETIC VALVE FOR TRANSLUMINAL DELIVERY

Appl. No.: Unknown A

Seguin, et al.
Atty Docket: CVALVE.006CP1

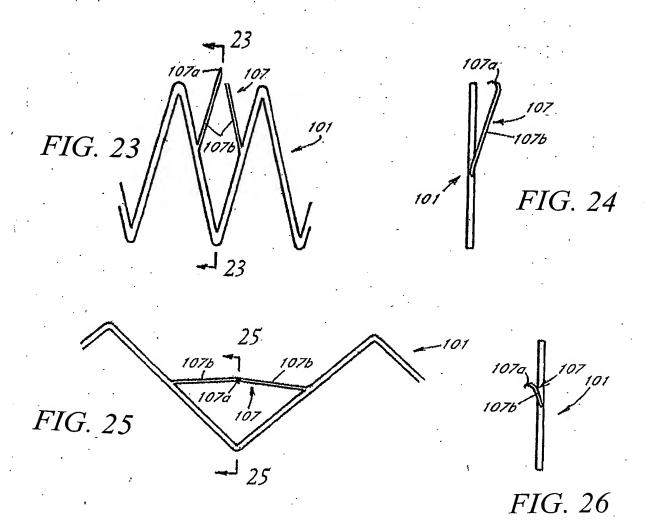

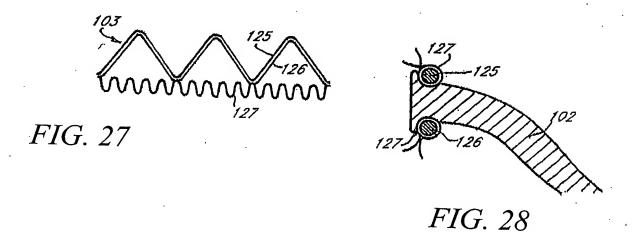

Atty Docket: `CVALVE.006CP1 Appl. No.: Unknown

11/38

FIG. 29






FIG. 30





108

FIG. 31




FIG. 32


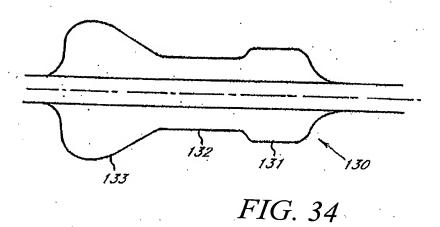


FIG. 33

Appl. No.: Unknown




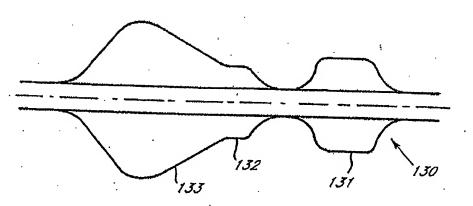



FIG. 35

Appl. No.: Unknown

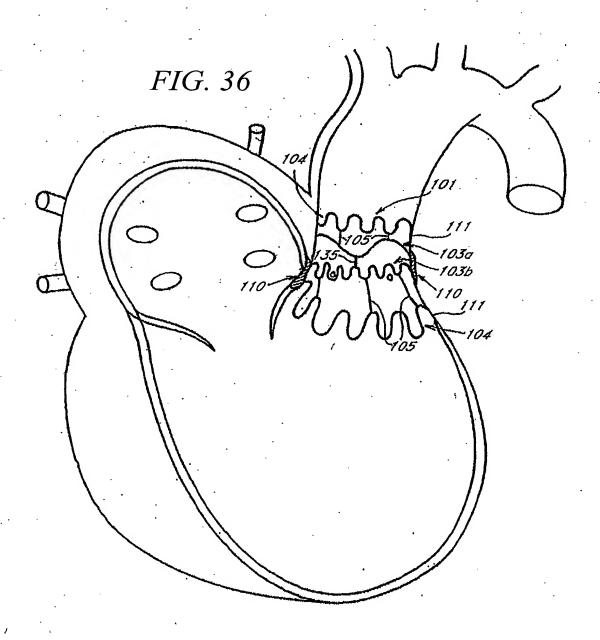

Appl. No.: Unknown

FIG. 37

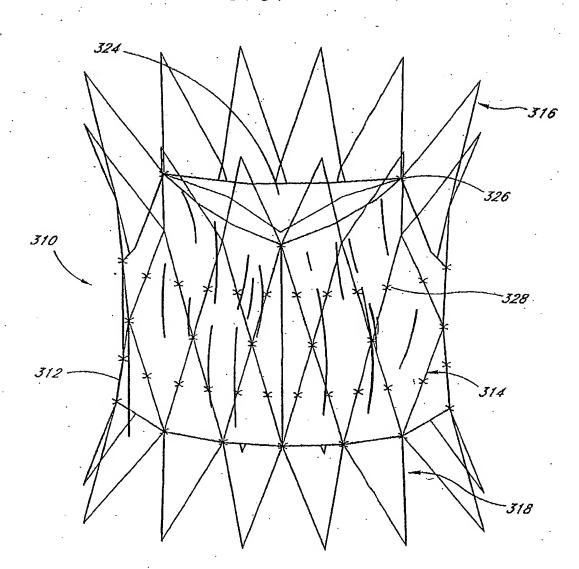

Appl. No.: Unknown

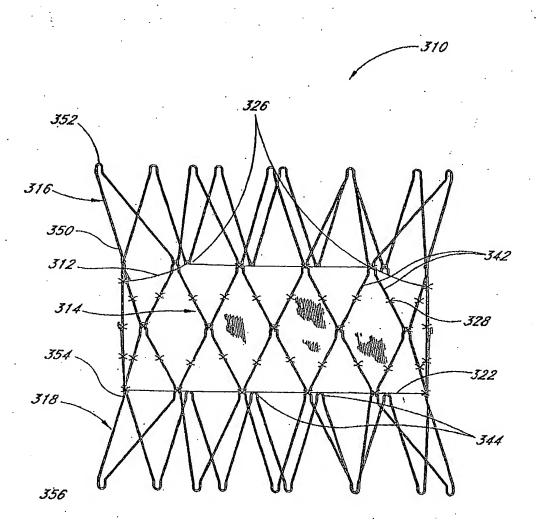


FIG. 38

Appl. No.: Unknown

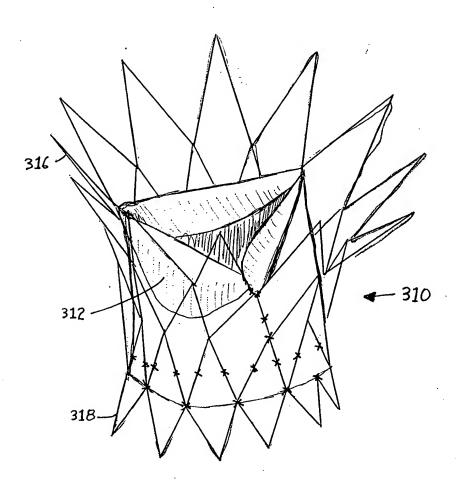


FIG. 39

Appl. No.: Unknown


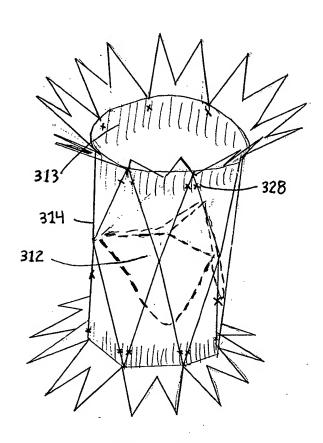


FIG. 40

Appl. No.: Unknown

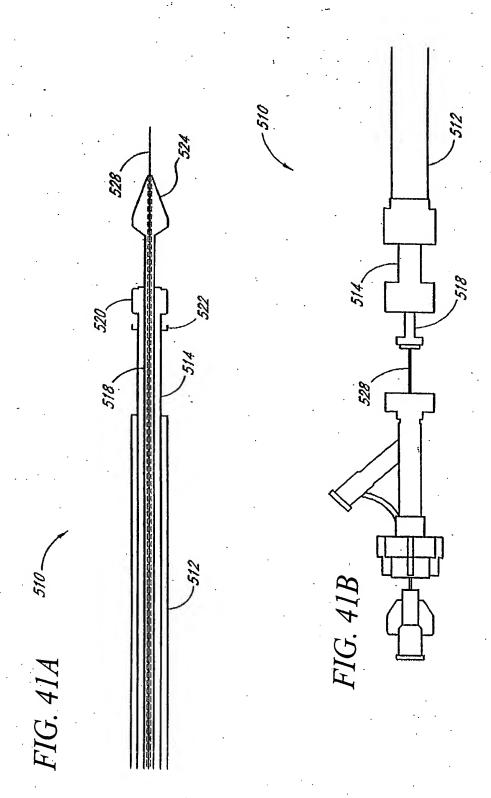

Appl. No.: Unknown

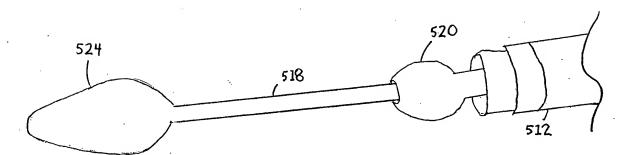


FIG. 42

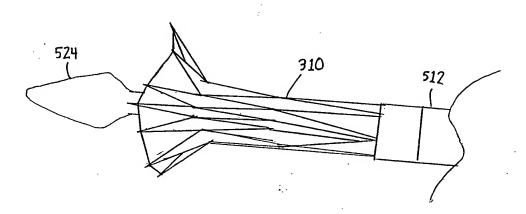
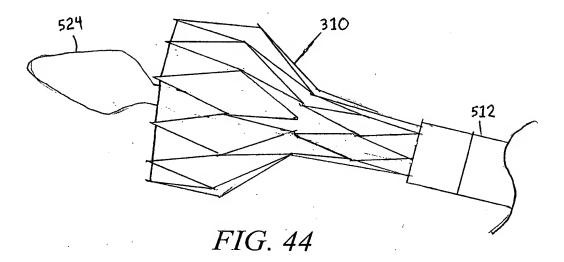


FIG. 43

Appl. No.: Unknown



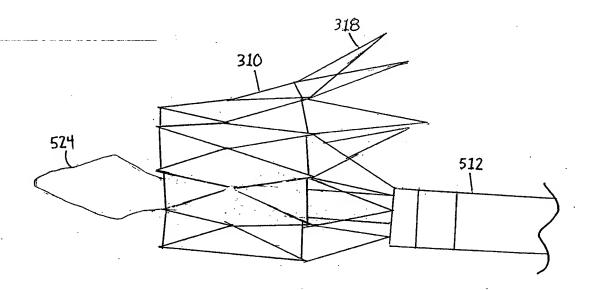
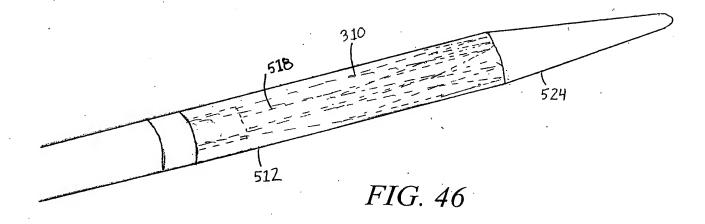


FIG. 45

Appl. No.: Unknown



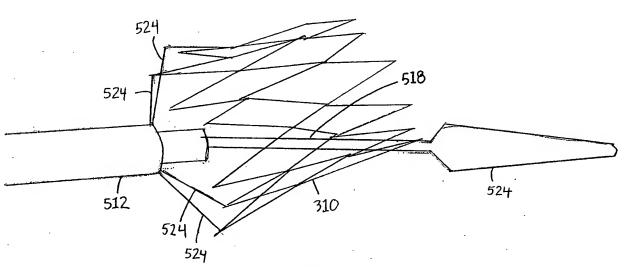


FIG. 47

Appl. No.: Unknown

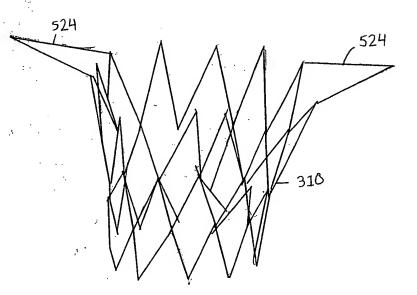


FIG. 48



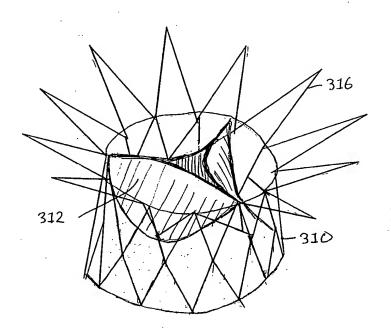



FIG. 49

Appl. No.: Unknown

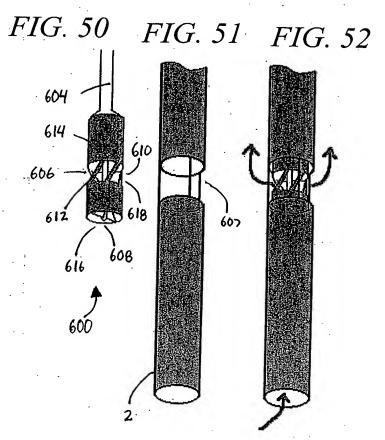

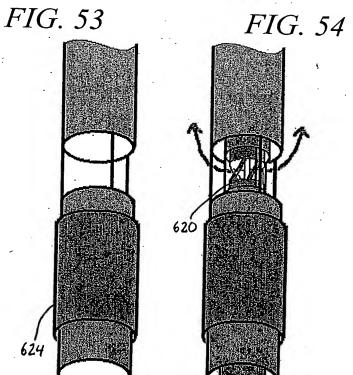

Appl. No.: Unknown

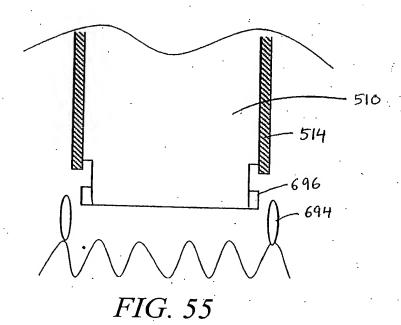

Appl. No.: Unknown

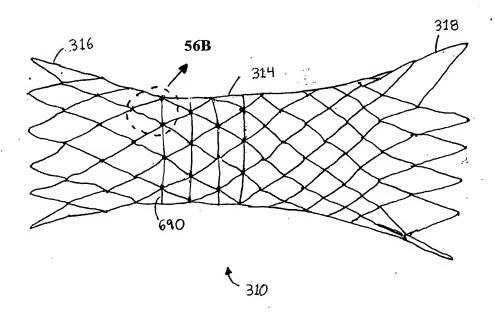


FIG. 56A




FIG. 56B

Appl. No.: Unknown

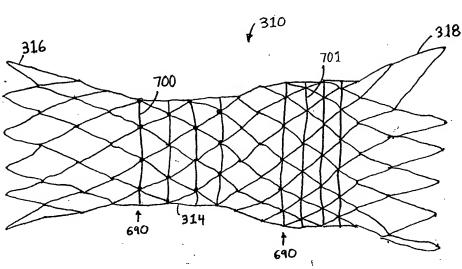


FIG. 57

Appl. No.: Unknown

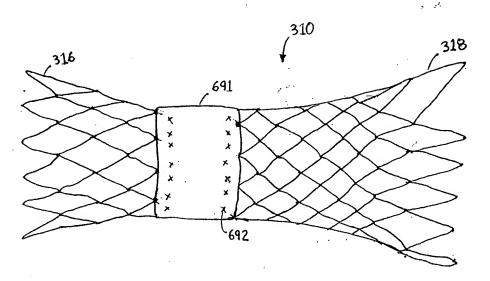


FIG. 58

Appl. No.: Unknown

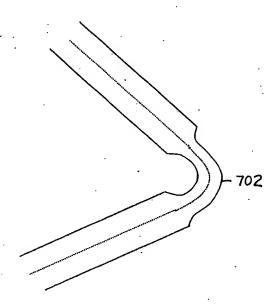


FIG. 59







FIG. 60

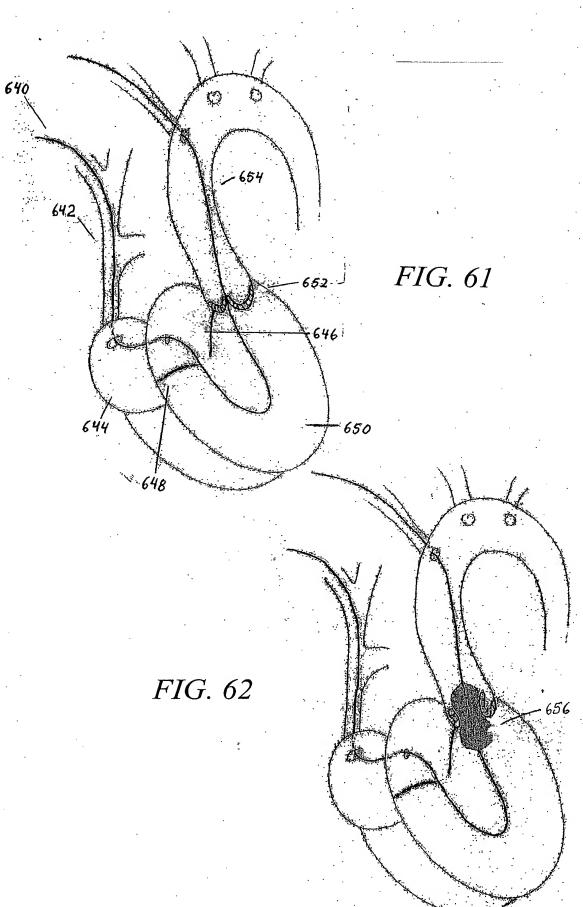


Appl. No.: Unknown

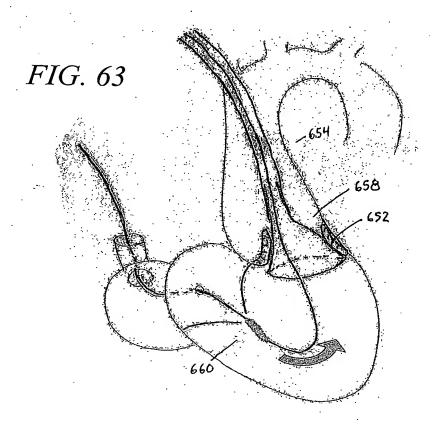

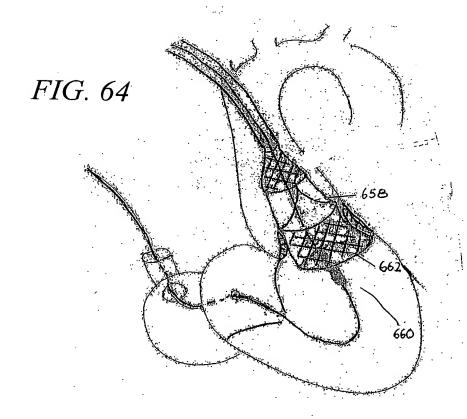

Appl. No.: Unknown

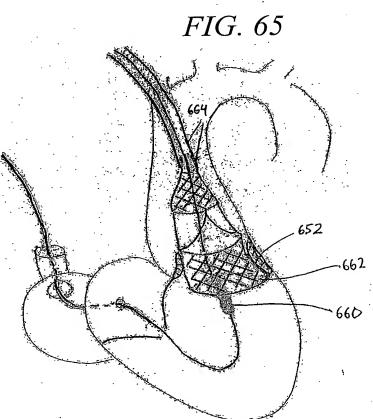

Appl. No.: Unknown


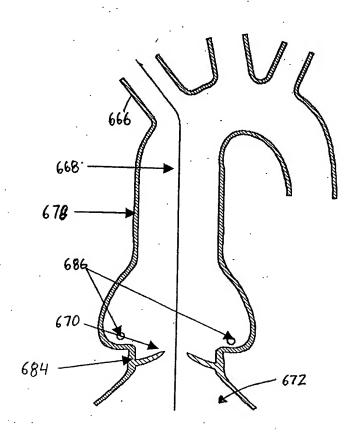


FIG. 67



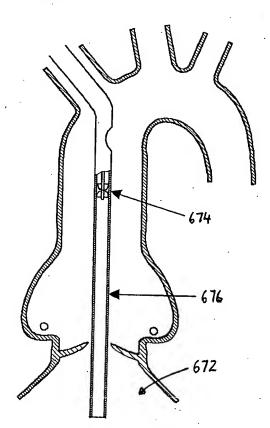

Appl. No.: Unknown



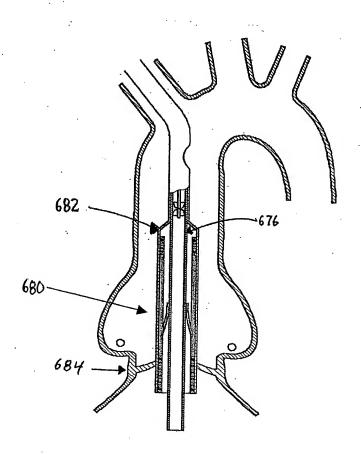


FIG. 68





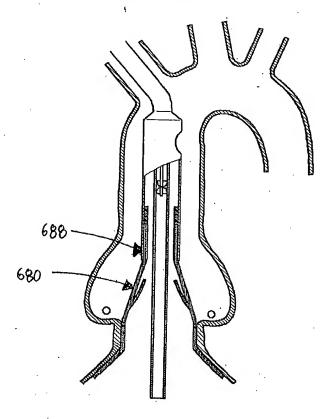

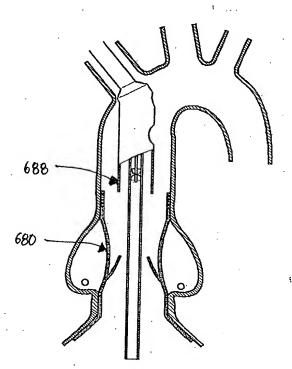

PROSTHETIC VALVE FOR TRANSLUMINAL DELIVERY

Seguin, et al.
Atty Docket: CVALVE 006CP1 Appl. No.: Unknown

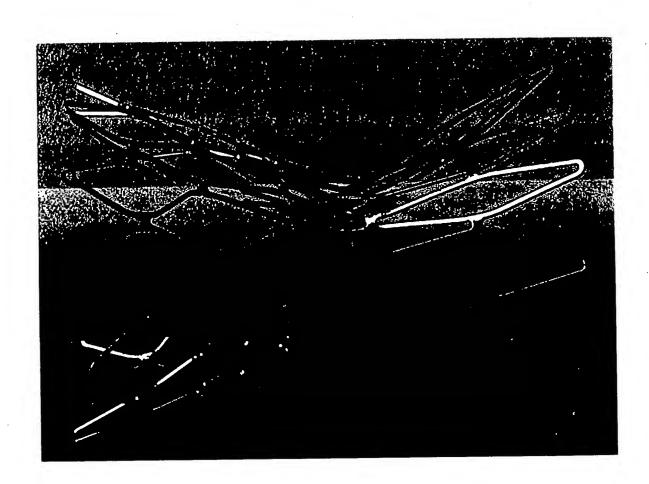


FIG. 71

PROSTHETIC VALVE FOR TRANSLUMINAL DELIVERY

Appl. No.: Unknown

Seguin, et al.
Atty Docket: CVALVE.006CP1

36/38

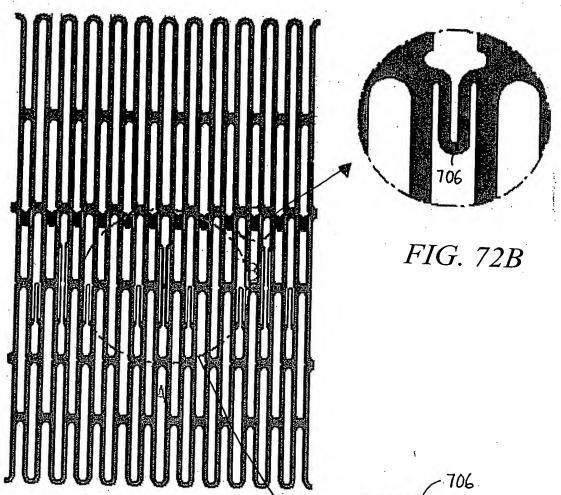


FIG. 72A


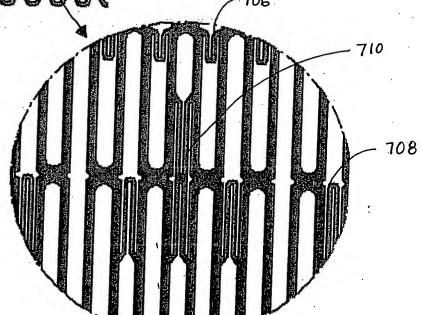


FIG. 72C

PROSTHETIC VALVE FOR TRANSLUMINAL DELIVERY Seguin, et al.

Appl. No.: Unknown Atty Docket: CVALVE.006CP1

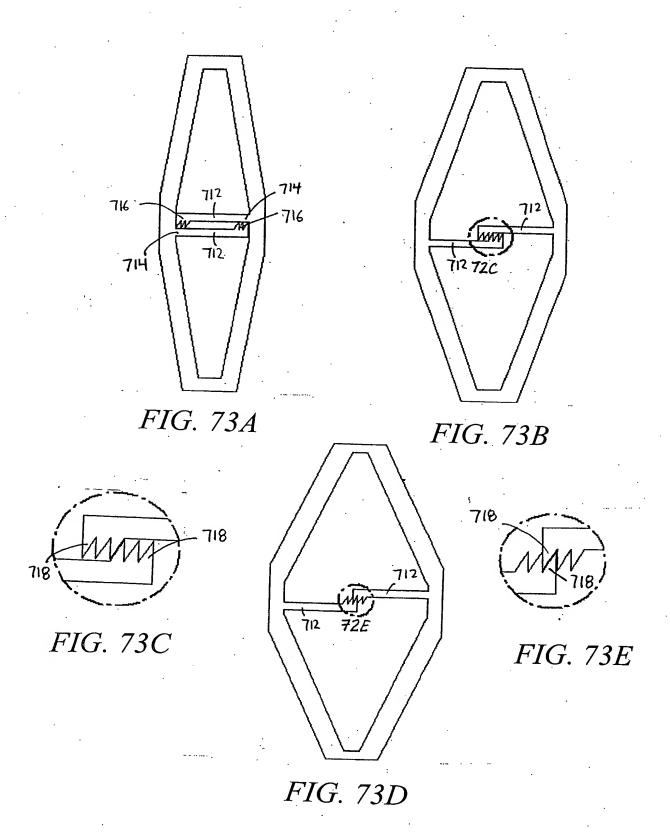

Appl. No.: Unknown

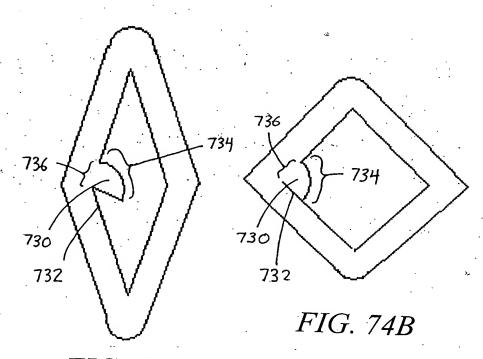


FIG. 74A

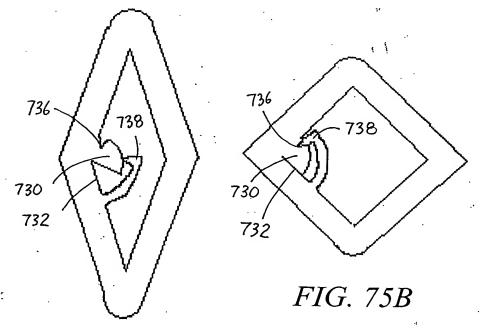


FIG. 75A